

Figure 1. *In vitro* bupivacaine release from collagen device over time.

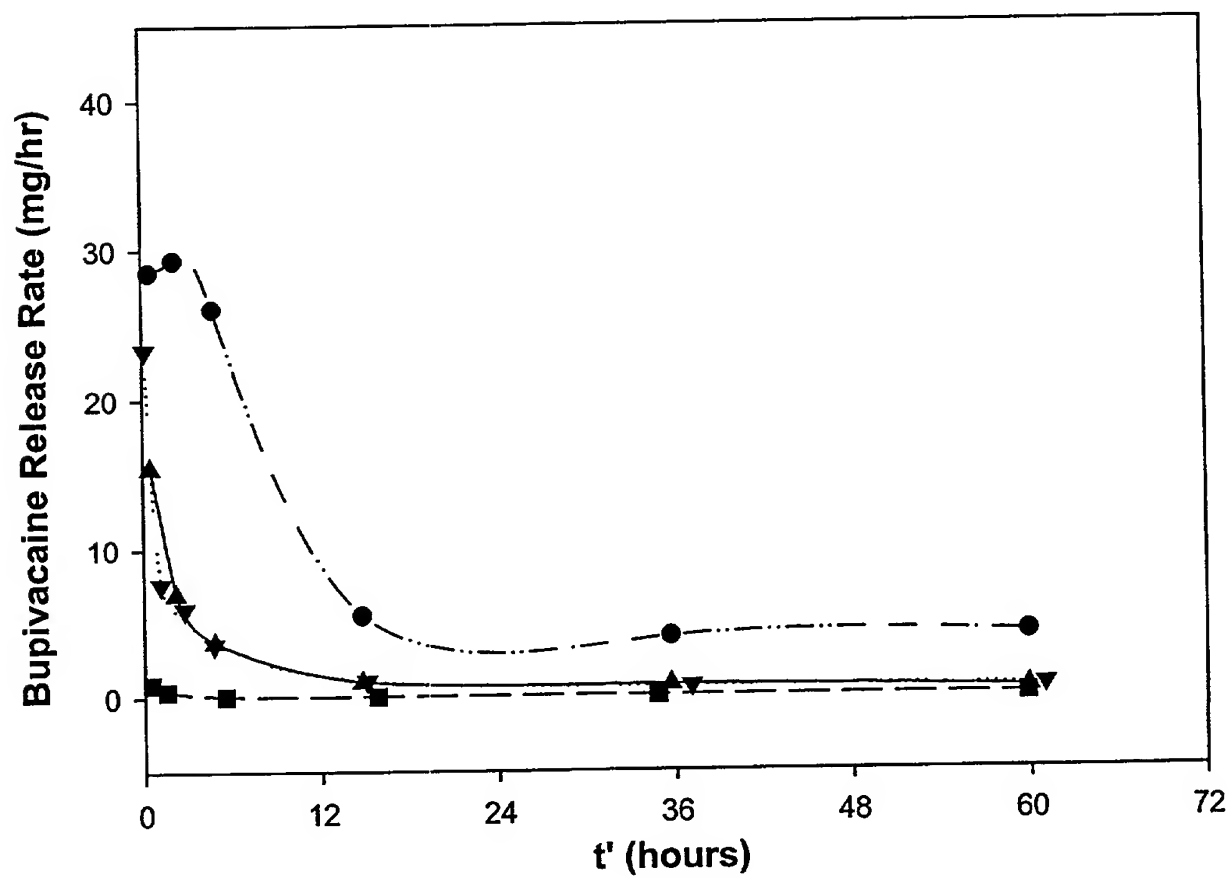


Figure 2. Bupivacaine Release Rate

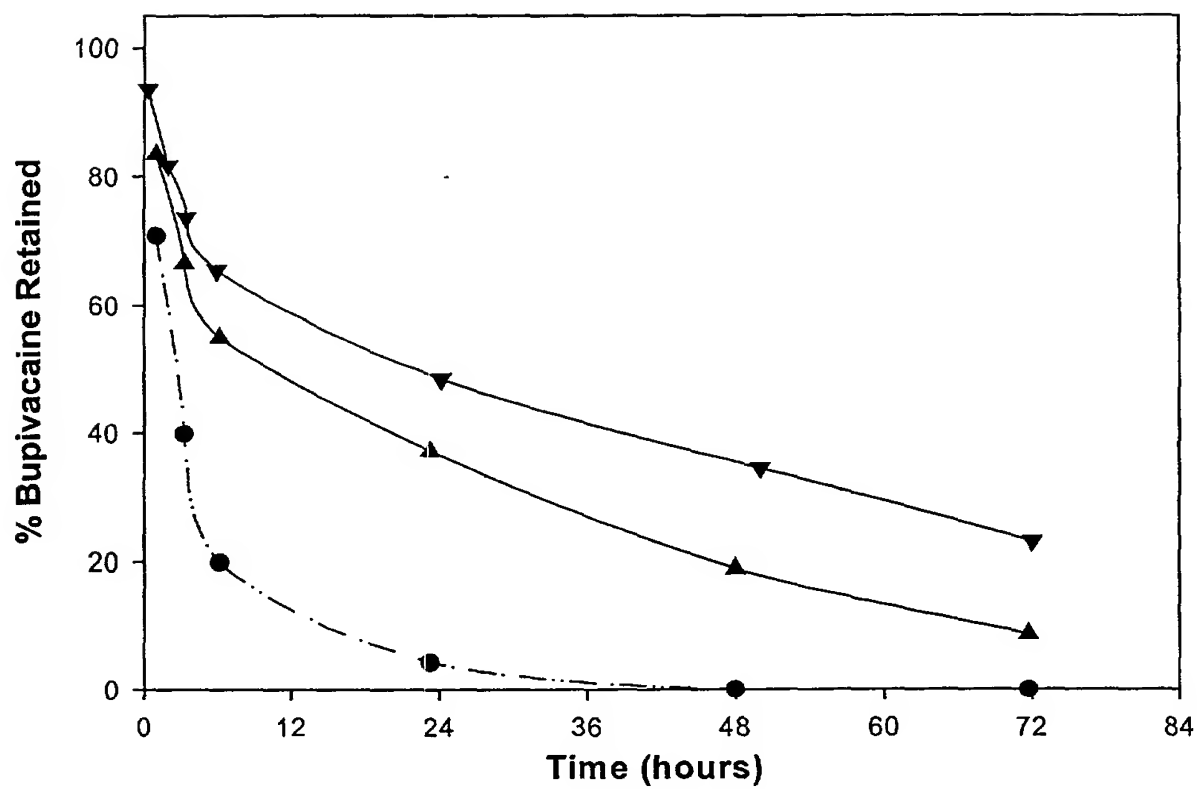


Figure 3. Percent Bupivacaine Retained in Sample